



# Assemble and disassemble of the products

Some instruments include two or several parts. Before cleaning and disinfection they shall be disassembled and before sterilization - assembled.

## Implant drivers HE MP


Assemble the implant driver HE with appropriate screwdriver SITHE before sterilization. Use for implant insertion via carrier HFCM and for removal of HFCM. After use, disassemble the implant driver HE for cleaning and disinfection.

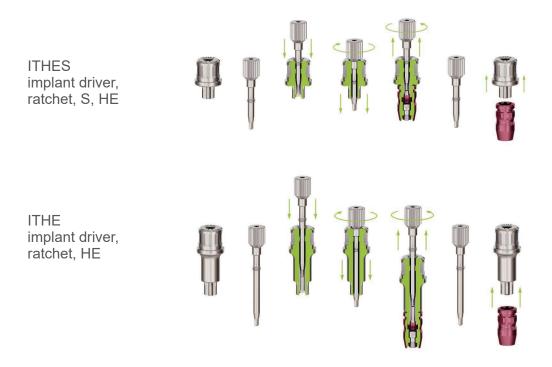


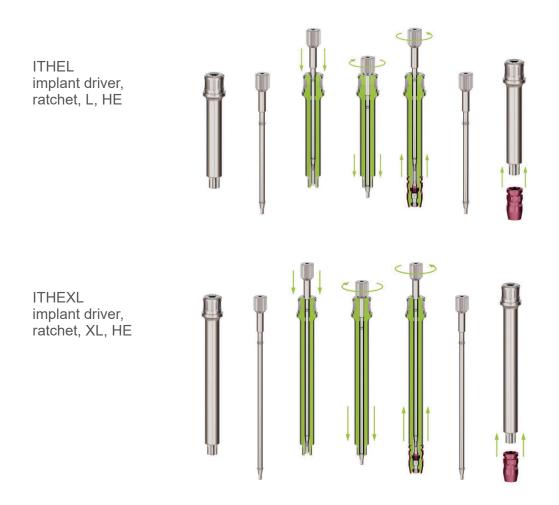

## Implant drivers MP

Assemble implant driver M with appropriate screw SITM before sterilization. Use for implant insertion. After use, disassemble implant driver M for cleaning and disinfection.

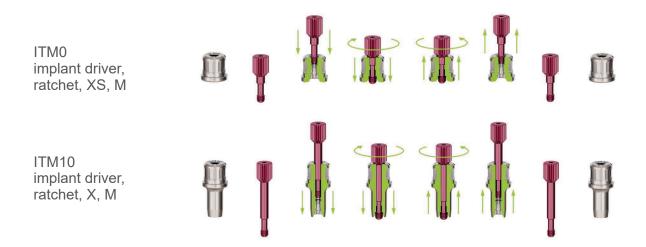


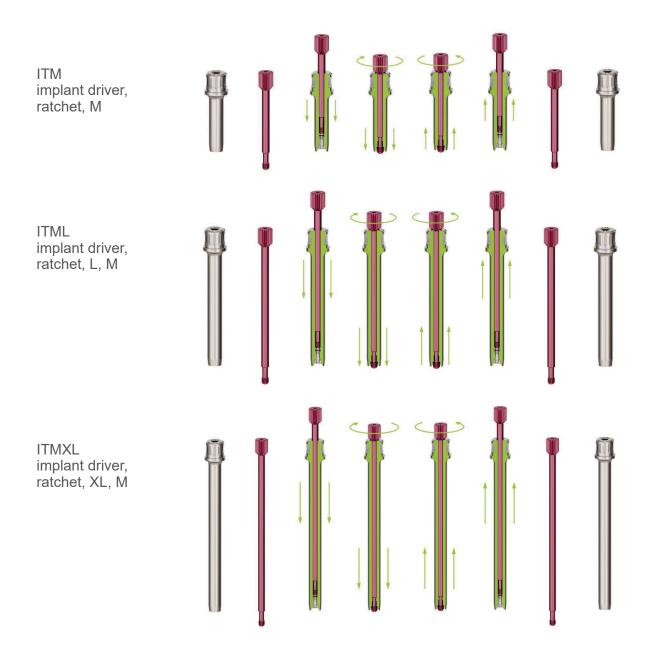

#### Implant drivers S

Assemble implant driver S with appropriate screw SITMS before sterilization. Use for implant insertion. After use, disassemble implant driver S for cleaning and disinfection.

ITMS implant driver, ratchet, S, S

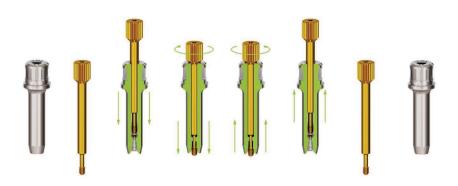



## Wrenches U

RW - ratchet wrench. Assemble the instrument before sterilization and disassemble after use, for cleaning and disinfection



Some instruments can be used together. After use, they must be disassembled, then cleaned, disinfected, sterilized separately.



ET + drills - all drills can be used with drill extension tool ET, for handpiece



ETEAO + drills - all drills can be used with drill extension tool ETEAO, for AO connection



ETH + drills - all drills can be used with surgical handle, handpiece.



ETAO+AO connection instruments: ITAO, ITEAO, ITEAOK, ITHEAO, SDAO, ETEAO can be used with surgical handle, AO. Pull quick change interface (as shown) to insert or to take out instrument.

# Guided surgery **U**

Drill stops + drills - all drills can be used with drill stops. Drill stops are different diameter (S1, S2, S3) and length (2 mm, 4 mm, 6 mm, 8 mm, 10 mm, 12 mm, 14 mm, 16 mm).

